BIOVIRIDIAN

Excellence in HPLC-MS Analysis

CERTIFICATE OF ANALYSIS

Web Verification Code: **COA2667**

Sample Received: **January 7, 2026** | COA Issued: **January 10, 2026**

PRODUCT INFORMATION

Vendor: **BioMyst Labs**

Sample Name: **Glow 50, 10, & 10 mg**

Sample Type: **Blue lyophilized powder**

Lot Number: **NA**

MW: **403.3, 1419.1 & 4964.1 g/mol**

ANALYTICAL METHODS

Identity: Confirmed via MALDI–MS
Purity: RP-HPLC (214 nm)
Content: HPLC quantitation


TEST RESULTS

Specification	Result	Method	Status
Identity: GHK-Cu, BPC-157 & TB-500	**GHK-Cu, BPC-157 & TB-500**	**MALDI-MS**	✓ Conforms
Content	**51.31, 10.11, & 9.76 mg**	HPLC Quantitation	✓ Conforms
Purity	**99.8 %**	RP-HPLC (214 nm)	✓ Conforms


ANALYTICAL DATA


HPLC Chromatogram (Retention Time: 2.117, 5.78,& 5.98 min)



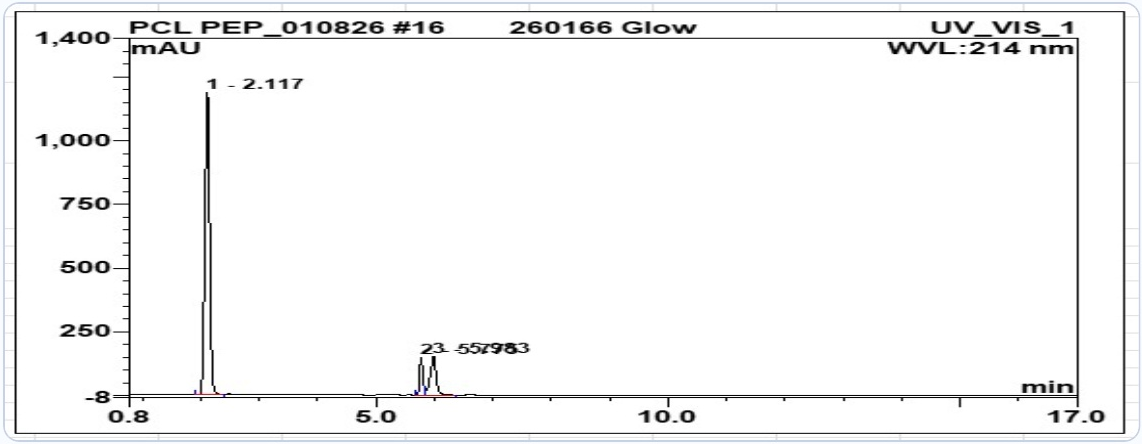

Mass Spectrum (MALDI-MS)

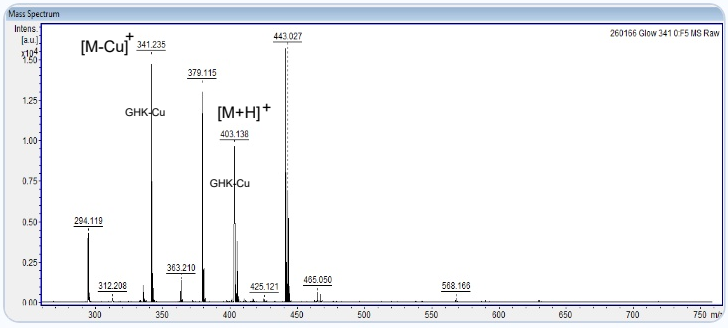

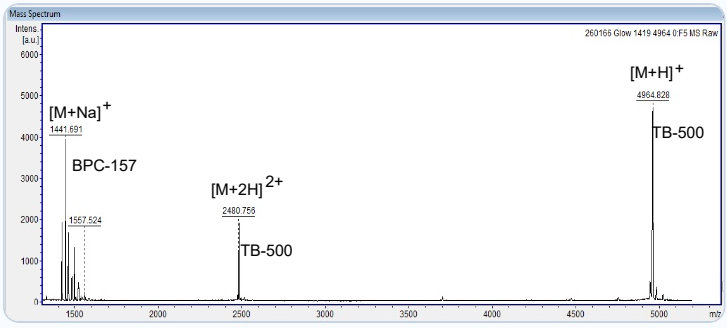

Certification: This COA confirms that the tested material meets or exceeds Bioviridian's analytical quality specifications for peptide research use.

Visit: https://bioviridians.com/coa-search.html

Shane Straight

Shane Straight, M.S.
Principal Chemist, Bioviridian Inc.